



(19) World Intellectual Property Organization  
International Bureau



PCT

(10) International Publication Number  
WO 02/38207 A1

(51) International Patent Classification: A61M 15/00, D02B 11/00

(71) Inventor and  
(72) Inventor/Applicant (for US only): POLLOCK, Neil  
(GB/GB); 20 Coombe Road, Rayson, Here SG9 2DW  
(GB)

(81) International Application Number: PCT/GB01/04964

(74) Agents: GILL, JENNINGS & EVERETT; Broadgate House,  
7 Eldon Street, London EC2M 7LH (GB)

(52) International Filing Date:  
7 November 2001 (07.11.2001)

(82) Designated States (abstract): AE, AG, AL, AM, AT, AU,  
AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU,  
CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GR, GT, HK,  
HU, IL, IN, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LU,  
LV, LY, MA, MD, MG, MK, MN, MW, MX, MY, NZ, OM, PA,  
PE, PG, PH, PL, PT, RU, SA, SD, SG, SI, SK, SL, TH, TM,  
TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.

(53) Filing Language: English

(54) Publication Language: English

(56) Priority Date:  
0010043.2 13 November 2000 (13.11.2000) EP


(77) Applicant (for all designated States except US): THE  
TECHNOLOGY PARTNERSHIP PLC (GB/GB);  
Medema Science Park, Cambridge Road, Medema,  
Rayson, Hertfordshire SG9 6EB (GB)

(84) Designated States (epilogue): ARIPO patent (GH, GM,  
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian  
patent (AM, AZ, BY, EG, GZ, MD, RU, T1, TM), European  
patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE,  
IT, LI, LU, MC, NL, PT, SE, TR), OAPI patent (BF, BI, CF,  
CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD,  
TG).

[Continued on next page]

(54) Title: AEROSOL DRUG-DISPENSING WITH MEMBRANE FOR CONTROLLING VACUUM DURING DISPENSING

(57) Abstract: An aerosol drug-dispensing device (25) provides a measured dose of a pharmacologically active liquid (7) to a holding reservoir (14), which includes a perforate membrane (14) from which the dose is dispensed as an aerosol spray. The holding reservoir (14) is located in a chamber (1) which has a movable surface in the form of a resilient diaphragm (15) which is stretchable to vary the volume of, and thus adjust the pressure in, the chamber (1) to provide a pressure differential across the resilient diaphragm (15) during actuation of the perforate membrane (14) such that the pressure within the holding reservoir (14) is less than the ambient pressure on the opposite side of the perforate membrane (14). A control device (13, 5, 19) is arranged to control the stretching of the resilient diaphragm (15) and thus the generation of the differential pressure across the perforate membrane (14).

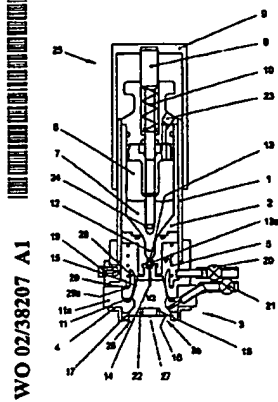

WO 02/38207 A1

WO 02/38207

PCT/GB01/04964

AEROSOL DRUG-DISPENSING WITH MEMBRANE FOR CONTROLLING VACUUM DURING DISPENSING

This invention relates to aerosol drug dispensing devices and, in particular, to those devices in which pharmacologically active liquid is provided to a holding reservoir from which the dose is then dispensed as an aerosol spray.

Prior known aerosol drug dispensing devices have used a number of different means for creating a negative pressure behind a perforate membrane which acts as part of a spray head. In order that a dose of pharmacologically active liquid can be dispensed as a spray, the perforate membrane must be actuated to cause liquid flow through the perforate membrane.

Previously, the perforate membrane has been actuated by vibrating means and the pressure on the liquid side of the perforate membrane altered by means such as a pump or an expanding syringe mechanism. These methods have proved to be complex and the devices are difficult to manufacture.

Our earlier international patent application, WO95/15822, discloses a dispensing apparatus having a perforate membrane through which droplets are dispensed. The perforate membrane is provided with a number of perforations having a reverse taper, namely a larger cross-sectional area at that face of the membrane away from which liquid droplets emerge than at the opposite face of the membrane, from which opposite face liquid flows in use to replace that in the emerging droplet spray.

The present invention aims to overcome the above problems.

According to the present invention, there is provided an aerosol drug dispensing device in which a measured dose of a pharmacologically active liquid is provided to a holding reservoir from which the dose is then dispensed as an aerosol spray, the holding reservoir including a perforate membrane from which the dose is dispensed by actuation of the perforate membrane to cause liquid flow through the perforate membrane, the perforate membrane having perforations having a reverse taper, namely a larger cross-sectional area at that face of the membrane away from which liquid droplets emerge than at the opposite face of the membrane, characterised in that:

The holding reservoir is disposed in a chamber having a movable surface in the form of a resilient diaphragm which is stretchable to vary the volume of, and thus adjust the pressure in, the chamber to provide a pressure differential across the resilient diaphragm during actuation of the perforate membrane such that the pressure within the holding reservoir is less than the ambient pressure on the opposite side of the perforate membrane;

a control device is arranged to control the stretching of the resilient diaphragm and thus the generation of the differential pressure across the perforate membrane.

WO 02/38207

PCT/GB01/04964

In this way, the differential pressure can simply and accurately be controlled such that the required pressure differential is easily maintained.

Preferably, the resilient diaphragm is formed from an elastomeric material such as rubber.

Preferably, the chamber contains one or more valves for controlling the inlet and/or outlet of fluids from the chamber.

The control device may be a reciprocating plunger which is connected to the resilient diaphragm substantially at the centre.

Preferably, the resilient diaphragm is clamped by a spray head assembly substantially at its outer edge. Sealing means such as an O-ring may be provided to ensure no fluid flows past the resilient diaphragm.

An embodiment of the present invention will now be described with reference to the accompanying drawings, in which:

Fig. 1 shows a cross sectional side view of a device according to the present invention;

Figs. 2 to 6 show successive stages during operation of the device of Fig. 1;

Fig. 7 shows a trigger circuit for controlling the dispensing of the pharmacologically active liquid; and

Figs. 8a and 8b illustrate, in section, preferred forms of the perforate membrane for the device of Fig. 1.

As can be seen from Figs. 1 to 6, a drug dispensing device 25 forming part of a drug delivery system has a hollow casing 1 in which a reservoir body 2 is slidably mounted. A spray head mounting assembly 3 is attached to one end of the casing 1, the mounting assembly 3 comprising spray head assembly 3a, clamping means 4, diaphragm clamp 11a and seal 17. A main return spring 5 is provided between a recess 29 in the casing 1 and the reservoir body 2 to support the reservoir body 2, biased towards its rearmost position (as shown), within the casing 1. The reservoir body 2 is movable between a first and second position within the casing 1.

The reservoir body 2 has a reservoir cavity 6 in which a liquid drug 7 is stored and which can be topped-up via a re-fill port 23. A plunger 8 is provided within the reservoir body 2 and extends out of the upper (as shown in the figures) end of the reservoir body 2, such that it engages with a cap 9 which covers the top of the device 25. A plunger return spring 10 is provided which extends from the reservoir body 2 and biases the plunger 8 out of the reservoir cavity 6.

A metering cavity 12 is provided at the lower end of the reservoir cavity 6 and the metering cavity 12 is in fluid communication, via a one-way ball valve 13, with a dispensing conduit or tube 14 provided within the lower end of the reservoir body 2. An

elastomeric diaphragm 15 is provided around the lower portion of the reservoir body 2 and is joined at its outer edge to the casing 1 by diaphragm clamp 11a and a seal 11, which is an O-ring, to define, together with the reservoir body 2 and the casing 1, a chamber V1.

The spray head mounting assembly 3 is provided with an outlet 26 covered by a membrane 16 which, together with the lower portion of the reservoir body 2, the spray head mounting assembly 3 and the elastomeric diaphragm 15, defines a chamber V2. The membrane 16 is retained by a seal 17 and is provided with a perforate portion 27 over which a holding reservoir 18 is provided and which can receive liquid drug 7 through the dispensing conduit or tube 14 in use. The perforate portion 27 of the membrane 16 has perforations 50 (see Figs. 6a and 6b) of a reverse taper and this is described in greater detail with reference to Figs 6a and 6b.

The spray head mounting assembly 3 is provided with a damping inlet valve 19 leading into the chamber V1, a first one-way exhaust valve 20 from the chamber V1 and a second one-way exhaust valve 21 from the chamber V2.

Fig. 1 shows the device 25 at rest prior to metering a predefined dose of drug 7 into the holding reservoir 18. In this state, both the main return spring 5 and the plunger return spring 10 are extended so that the reservoir body 2 and the plunger 8 have been pushed fully upwards against physical stops (not shown).

The elastomeric diaphragm 15 is stretched from its normally flat state and acts as a flexible wall, separating the two chambers V1 and V2. These chambers are initially at ambient pressure and the perforations 50 in the perforate portion 27 of membrane 16 are dry and open.

The operation of the device shown in Fig. 1 will now be described with reference to Figs. 2 to 6.

To initiate operation of the device 25, the cap 9 is pressed downwards 9a (see Fig. 2). The reservoir body 2 and the plunger 8 are moved downwards at approximately the same rate, compressing the main return spring 5 until the reservoir body 2 reaches physical stops 28. At this stage the force exerted on the plunger return spring 10 is less than its preload. The lower end of the dispensing conduit or tube 14 is now positioned close to the inner surface of the membrane 16.

The reservoir body 2 forms an air-tight sliding seal with the casing 1. Therefore, as the reservoir body 2 descends, air is displaced from the chamber V1, through the first one-way exhaust valve 20 and the elastomeric diaphragm 15 returns towards its relaxed, almost flat state. At the same time, air is displaced from the chamber V2 through the second one-way exhaust valve 21, through the damping valve 19, and through the perforate portion 27 of the membrane 16.

3

pressures generated in the chambers V1, V2 and by tension in the elastomeric diaphragm 15.

However, when the damping valve 19 is slightly open, it will allow air to enter into, and conversely exhaust from, the chamber V1 at a rate determined by the restoring force of the main return spring 5. Therefore, as the main return spring 5 pushes the reservoir body 2 upwards 2a, the volume of chamber V1 expands at a controlled rate until the reservoir body 2 reaches a predefined physical stop (not shown) (see Fig. 6).

The main return spring 5 also causes the elastomeric diaphragm 15 to stretch at a controlled rate which, in turn, causes the volume of the chamber V2 to expand at a controlled rate. The pressure within the chamber V2 behind the spray head assembly 3a therefore reduces at a controlled rate.

The physical stop (not shown) for the upward movement of the reservoir body 2 limits the extension of the stretched elastomeric diaphragm 15 and defines the final volume change of the chamber V2 and thus the target negative pressure achieved in V2. At this stage, the pressure in the chamber V1 is at ambient pressure.

Therefore, the net result is that the target (operating) negative pressure, which is close to the bubble point pressure for the spray head assembly 3a (the bubble point pressure being the pressure differential at which air bubbles enter the chamber V2 through the perforations 50 in the perforate portion 27, by overcoming the surface tension of the meniscus of liquid drug), can be reached at a controlled rate without air being ingested through the membrane 16.

If the negative pressure in the chamber V2 is generated too quickly, i.e. by opening the damping valve 19 too far, then the surface tension of the liquid drug covering the perforations in the perforate portion 27 of the membrane 16 will be overcome. Air will then be ingested rapidly through the perforate portion 27, hence cancelling the negative pressure in the chamber V2. In the absence of a negative pressure, the drug dispensing device 25 will not generate a spray.

It should be noted that the rate of air admission and exhaustion through damping valve 19 is much less than the rate of exhaustion through the first one way exhaust valve 20.

An electronic control circuit 30 as shown in Fig. 7 triggers the delivery of the liquid drug through the perforate portion 27 of the membrane 16 by controlling membrane actuating means (not shown) such as piezoelectrically actuated vibrating means. The control system uses a small hot wire anemometer 39 to monitor air flow into the drug delivery system. The anemometer 39 senses when a patient is inhaling and trying to trigger the spray head delivery.

5

As can be seen in Fig. 3, once the reservoir body 2 has reached its physical stops 28, further depression of the cap 9 compresses the plunger return spring 10. This pushes the plunger 8 into the metering cavity 12 (see Fig. 1). The plunger 8 is provided with a plunger seal 24 which engages with the side wall 12a of the metering cavity 12 to form a seal therewith. This traps a metered dose of the liquid drug 7 in the metering cavity 12. The sealing pressure of the plunger seal 24 against the side-wall 12a of the metering cavity 12 is greater than the sealing pressure of the elastomeric ball valve 13 against the ball valve seat 13a. Therefore, as the plunger 8 is depressed further, the trapped dose of liquid drug 7 is displaced from the metering cavity 12 past 13b the one-way elastomeric ball valve 13, through the dispensing conduit or tube 14 and into the holding reservoir 18. The holding reservoir 18 has a side-wall 22 which is either coated with or formed of PTFE. In this configuration, all of the perforations 50 in the perforate portion 27 of membrane 16 are now covered with liquid drug 7a.

Once the cap 9 is released, as shown in Fig. 4, the plunger return spring 10 starts to expand, pushing the plunger 8 out of the metering cavity 12, thus creating a partial vacuum in the metering cavity 12. The elastomeric ball valve 13 remains closed. The plunger return spring 10 is strong enough to overcome this partial vacuum so as to push the plunger 8 clear of the metering cavity 12 until it reaches a physical stop (not shown). This partial vacuum pressure reduces as the plunger 8 is withdrawn 8b from the metering cavity 12 until the pressure drop across the plunger seal 24 exceeds the sealing pressure against the side-wall 12a of the metering cavity 12. A small amount of liquid drug 7 can then flow past the plunger seal 24 into the metering cavity 12 as the plunger 8 is withdrawn 8b. The main return spring 5 is able to extend, pushing the reservoir body 2 upwards as shown in Fig. 5. This then causes the chambers V1 and V2 to expand and the elastomeric diaphragm 15 to stretch.

Air cannot enter through the one-way valves 20, 21 or through the perforate portion 27 of membrane 16 as the perforations 50 are now covered by liquid drug 7a. The perforations 50 resist air ingress because of the surface tension of the liquid drug forming meniscus across the perforations 50 in the perforate portion 27 and therefore, as the chambers V1 and V2 expand, the pressures within those chambers decrease below ambient pressure. The reservoir body 2 continues to move upwards 2a until the restoring force of the main return spring 5 is stalled by the opposing forces created, in the main, by the negative pressures in the chambers V1 and V2 and by the tension in the elastomeric diaphragm 15.

When the damping valve 19 is fully closed, no air can enter the chamber V1 and so the main return spring 5 will not extend far before it is stalled by the negative

4

The maximum spring load of the plunger return spring 10 preferably should not exceed 20N. This therefore limits the force that a user must exert in order to operate the device.

The plunger return spring 10 is preloaded and this preload should be greater than the fully compressed load in the main return spring 5. This ensures that the reservoir body 2 is fully down against its physical stop 28 before the dose is metered into the holding reservoir 18. If the dose is metered from the dispensing aperture 14 when the reservoir body 2 is not fully down, all or part of the dose may miss the holding reservoir 18. The target negative pressure in the chamber V2 will then not be reached when the cap 9 is released because the perforations in the perforate portion 27 of the membrane 16 will remain dry and open.

As the plunger 8 is withdrawn 8b from the reservoir cavity 12 a partial vacuum is created between the closed one-way elastomeric ball-valve 13 and the plunger seal 24. The spring force range of the plunger return spring 10 must be sufficient to lift the plunger 8 out of the reservoir cavity 12 when the cap 9 when the cap is released, in order to create a pressure difference across the plunger seal 24 (between the liquid drug, 7 in reservoir cavity 6 and the elastomeric ball valve 13) which exceeds the sealing pressure of the plunger seal 24 against the side-wall 12a of the reservoir cavity 12. Liquid drug 7 is then able to flow past the plunger seal 24 and into the reservoir cavity 12 as the plunger 8 is withdrawn 8b. This has the advantage of minimising foam generation within the reservoir cavity 12 especially with liquid drugs containing surfactants as part of their formulation.

The spring force range of the main return spring 5 must be sufficient to lift the reservoir body 2 against the negative pressures generated within the chambers V1, V2, the stretching of the elastomeric diaphragm 15 and the friction of the sliding seal between the reservoir body 2 and the casing 1.

The maximum tension in the elastomeric diaphragm 15, which is achieved when the reservoir body 2 is at rest, must be high enough to maintain the target negative pressure within the chamber V2 without the elastomeric diaphragm 15 deforming under that negative pressure. This tensioned force must not be high enough to prevent the main return spring 5 from lifting the reservoir body 2 up against the predetermined physical stop during the generation of the negative pressures.

In summary, the extension force of the plunger return spring 10 is greater than the extension force of the main return spring 5 which is greater than the tensioned force of the elastomeric diaphragm 15.

From Fig. 7, it can be seen that the control circuit employs two operational amplifiers (op-amps) 31, 32, which can supply output voltages over the full power supply

6

range, i.e. between the supply voltage  $V_{cc}$  and ground GND. Op-amp 31 is in closed loop configuration with a Wheatstone bridge to maintain a constant resistance of the anemometer filament 39. The drive voltage 40 for the Wheatstone bridge is supplied to the op-amp 32 which is configured as a voltage comparator. The comparator is a switching device having a measurement input and a reference input. When the measurement voltage 33 is higher than the reference voltage 34, the output 35 from the op-amp 32 switches from GND to  $V_{cc}$ .

Circuits of this type are well known in anemometry. However the circuit of Fig. 7 shows a simple implementation of a circuit which can discriminate between high and low rates of change of air flow. The RC time constant used for the reference voltage 34 is set so that it can respond, in a damped manner, to slowly varying conditions such as changes in ambient conditions and to the normal slow breathing of a patient. Therefore, the reference voltage 34 is insensitive to fast rates of change in air flow during the patient inhalation cycle. The measurement voltage 33 at the comparator op-amp 32 is an attenuated signal from the Wheatstone bridge drive voltage 40, but does not have a long time constant filter and so reacts directly with the patient's inhalation.

If the patient inhales at a sufficiently high volume rate, then the measurement voltage 33 will exceed the reference voltage 34 due to the difference in the time constant of the reference and measurement voltages. In order for this to happen, a certain threshold of rate of change of air flow must be exceeded. When the measurement voltage 33 exceeds the reference voltage input 34, there will be a change in the voltage state at the output 35. Since the comparator circuit does not have any feedback, it is operating in a high gain mode and so has only two output states, 0v and  $V_{cc}$ . Thus, it is possible to couple this circuit directly to TTL logic devices.

Two variable resistors 36, 37 are provided within the control circuit 30. The variable resistor 36 in the comparator is used to adjust the level of attenuation applied to the measurement voltage 33, which sets the sensitivity of the circuit to the rate of change of patient's inhalation. The second variable resistor 37, in the Wheatstone bridge, is provided to set the temperature of the anemometer filament 39 and is used to set the minimum rate of change of air flow that the circuit can detect. Thus, these adjustments allow a high degree of flexibility in the installation of the anemometer as a breath trigger device.

A field effect transistor 38 is used to alter the reference ratio of the Wheatstone bridge thus enabling or disabling the air flow sensor via "ENABLE". In this way, the power consumption of the control circuit 30 is reduced, allowing the device to have a useful operating life when powered by batteries.

7

Figure 8a shows cross-sectional detail of a first example perforate membrane 16, which is operable to vibrate substantially in the direction of arrow 58 and which is suitable for use with the drug dispensing device 25 to produce fine aerosol sprays. In one embodiment, the membrane 16 comprises a circular layer of polymer which contains a plurality of tapered conical perforations 50. Each perforation 50 has openings 53 in the front exit face and openings 54 in the rear entry face, which perforations are laid out in a square lattice. Such perforations may be introduced into polymer membranes by, for example, laser-drilling with an excimer laser.

Figure 8b shows cross-sectional detail of a second example perforate membrane 2016, which membrane is operable to vibrate substantially and suitable for use with drug dispensing device 25 in the direction of arrow 58. The membrane is formed as a circular disc of diameter 8mm from electroformed nickel, and is manufactured, for example, by Stark Veco of Eerbeek, The Netherlands. Its thickness is 70 microns and is formed with a plurality of perforations shown at 2050 which, at front face 2051, are of diameter shown at "a" of 120 microns and at rear face 2052 are of diameter shown at "b" of 30 microns. The perforations are laid out in an equilateral triangular lattice of pitch 170µm. The profile of the perforations varies smoothly between the front and rear face diameters through the membrane thickness with substantially flat "sand" regions (shown at "c") of smallest dimension 50µm in front face 2051.

20

8

## CLAIMS

1. An aerosol drug dispensing device in which a metered dose of a pharmacologically active liquid is provided to a holding reservoir from which the dose is then dispensed as an aerosol spray, the holding reservoir including a perforate membrane from which the dose is dispensed by actuation of the perforate membrane to cause liquid flow through the perforate membrane, the perforate membrane having perforations having a reverse taper, namely a larger cross-sectional area at that face of the membrane away from which liquid droplets emerge than at the opposite face of the membrane, characterized in that:

the holding reservoir is disposed in a chamber having a movable surface in the form of a resilient diaphragm which is stretchable to vary the volume of, and thus adjust the pressure in, the chamber to provide a pressure differential across the resilient diaphragm during actuation of the perforate membrane such that the pressure within the holding reservoir is less than the ambient pressure on the opposite side of the perforate membrane;

a control device is arranged to control the stretching of the resilient diaphragm and thus the generation of the differential pressure across the perforate membrane.

2. An aerosol drug dispensing device according to claim 1, wherein the resilient diaphragm is formed from an elastomeric material.

3. An aerosol drug dispensing device according to claim 2, wherein the elastomeric material is rubber.

4. An aerosol drug dispensing device according to any of claims 1 to 3, wherein the chamber contains one or more valves for controlling the inlet and/or outlet of fluids from the chamber.

5. An aerosol drug dispensing device according to any of claims 1 to 4, wherein the control device is a reciprocating plunger which is connected to the resilient diaphragm substantially at the centre.

6. An aerosol drug dispensing device according to any of claims 1 to 5, wherein the resilient diaphragm is damped by a spray head assembly substantially at its outer edge.

7. An aerosol drug dispensing device according to any of claims 1 to 6, including a sealing means to ensure that there is no fluid flow past the resilient diaphragm.

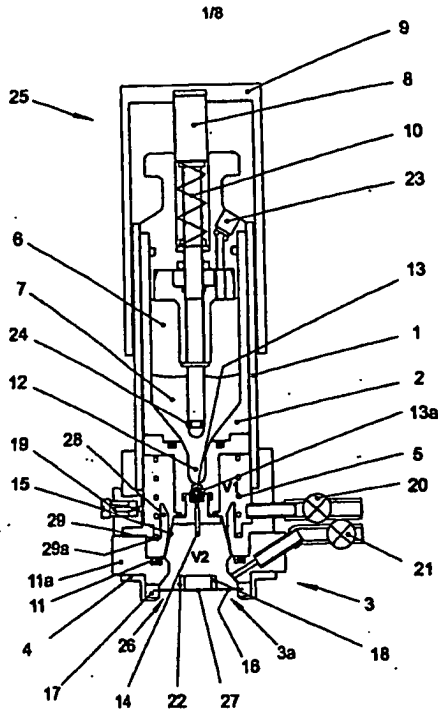


Figure 1

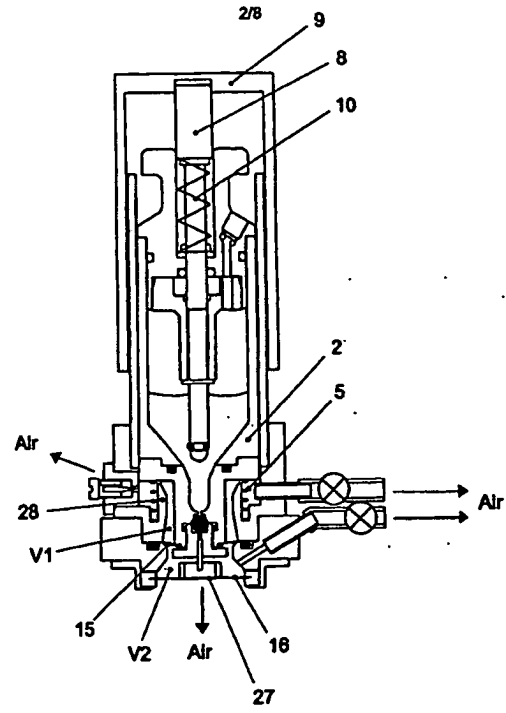


Figure 2

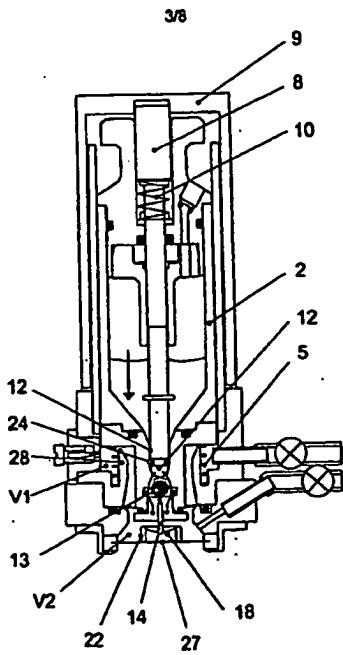


Figure 3

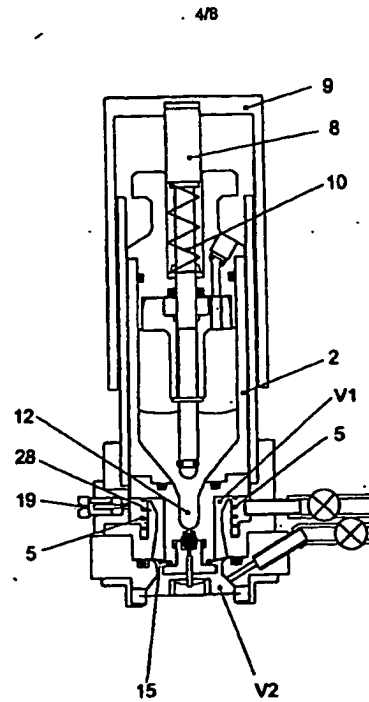


Figure 4

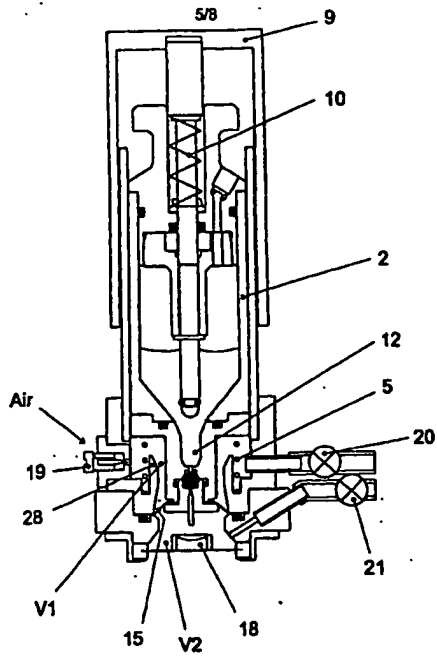


Figure 5

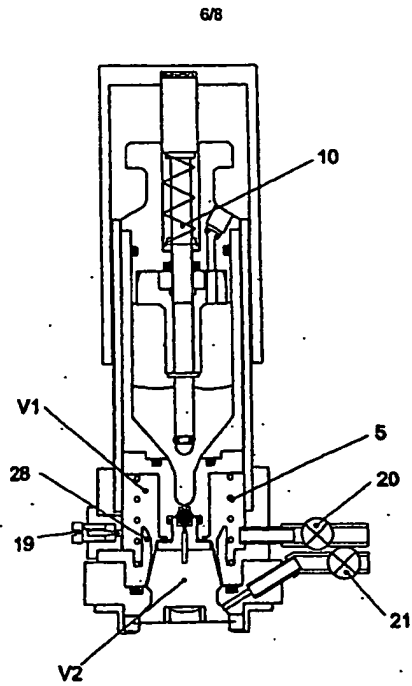


Figure 6

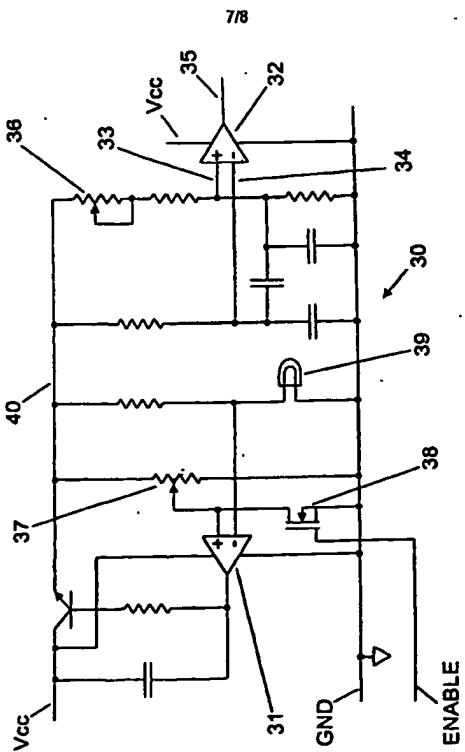


Figure 7

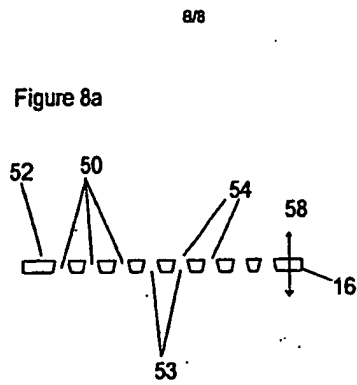


Figure 8a

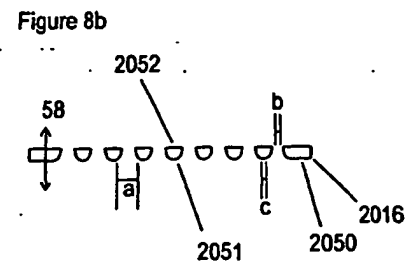


Figure 8b

INTERNATIONAL SEARCH REPORT		PCT/GB 01/04964
<b>A. CLASSIFICATION OF SUBJECT MATTER</b> IPC 7 A61R15/00 B05311/00		
According to International Patent Classification (IPC) to both national classification and IPC		
<b>B. FIELD SEARCHED</b> Abstracts disseminated according to classification system followed by examination according to IPC 7 A61R B05B		
Classifications searched other than abstracts (specify in the extent that such documents are available in the data provided)		
Electronic data base consulted during the international search process (state both end, where practical, search terms used) EPO-Internal, WPI Data, PAJ		
<b>C. DOCUMENTS CONSIDERED TO BE RELEVANT</b>		
Category	Character of document, with indication, where appropriate, of the relevant passages	Reference to date file
A	WO 95 15822 A (HUMBERSTONE VICTOR CAREY ; SAINT ANDREW JONATHAN (GB); TECHNOLOGY PA) 15 June 1995 (1995-06-15) cited in the application abstract	1
A	US 5 758 437 A (IVRI YEMUDA ET AL) 2 June 1998 (1998-06-02) abstract column 15, line 5 - column 17, line 5; figures 13-16	1
A	US 4 702 418 A (CARTER ROBERT E ET AL) 27 October 1987 (1987-10-27) abstract	1
<input type="checkbox"/> Further documents are listed in the continuation of box C. <input type="checkbox"/> Patent family members are listed in boxes.		
<b>D. Special categories of cited documents:</b>		
<input type="checkbox"/> Document relating to the general state of the art which has been mentioned in the particular abstract		
<input type="checkbox"/> Document published in an abstract international filing date		
<input type="checkbox"/> Document which has been cited in priority, claims or which is cited to establish the priority date of another invention or which is cited in the specification		
<input type="checkbox"/> Document relating to an end disclosure, use, modification or other event		
<input type="checkbox"/> Document published prior to the international filing date but later than the priority date claimed		
<input type="checkbox"/> Document published after the international filing date or priority date and not in conflict with the invention but cited to substantiate the principle or theory underlying the invention		
<input type="checkbox"/> Document of particular relevance; the abstract translation cannot be consulted and/or cannot be translated to verify an invention step which the document is taken into account in the art		
<input type="checkbox"/> Document of particular relevance; the abstract translation cannot be consulted in French or German; also within the document is combined with data or data other than character means, such as combined being referred to a general class of the art		
<input type="checkbox"/> Document number of the earlier patent family		
Date of the latest completion of the international search		Date of mailing of the international search report
25 February 2002		04/03/2002
Name and mailing address of the ISA European Patent Office, P.O. Box 1201 6000 Luxembourg Tel. (+352) 720 52-111; Fax (+352) 720 52-111 Fax (+352) 720 52-111		Authorised officer Nielsen, M

page 1 of 2

INTERNATIONAL SEARCH REPORT		PCT/GB 01/04964
<b>C. DOCUMENTS CONSIDERED TO BE RELEVANT</b>		
Category	Character of document, with indication, where appropriate, of the relevant passages	Reference to date file
A	US 6 062 212 A (BARRE'S PAUL ET AL) 16 May 2000 (2000-05-16) abstract	1
A	EP D 542 723 A (RESPAK PLC) 19 May 1993 (1993-05-19) abstract	1
A	US 5 823 434 A (COOPER GUY F) 20 October 1998 (1998-10-20) abstract	1

page 2 of 2

INTERNATIONAL SEARCH REPORT		PCT/GB 01/04964	
Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9515822	A 15-06-1995	AT 171654 T AU 687136 B2 AU 1195995 A BR 9408281 A CA 2176573 A1 CZ 9601681 A3 DE 69413708 D1 DE 69413708 T2 DK 732975 T3 EP 0732975 A1 ES 2123227 T3 WO 9515822 A1 JP 10502570 T US 5823428 A	15-10-1998 19-02-1998 27-06-1995 17-12-1996 15-06-1995 17-09-1997 09-11-1998 25-02-1999 21-06-1999 25-09-1996 01-01-1999 15-06-1995 10-03-1998 20-10-1998
US 5758437	A 02-06-1998	US 5586550 A AU 711059 B2 AU 7010096 A BR 9606617 A CA 2203926 A1 EP 0794433 A1 JP 10508251 T US 6085740 A WO 9707896 A1	24-12-1996 07-10-1999 19-03-1997 30-09-1997 06-03-1997 17-09-1997 19-08-1998 11-07-2000 06-03-1997
US 4702418	A 27-10-1987	MORE	
US 6062212	A 16-05-2000	GB 2272389 A AU 670342 B2 AU 534183 A CA 2144752 A1 CN 1101004 A DE 69316999 D1 DE 69316999 T2 EP 0582570 A1 ES 2113000 T3 FI 951490 A WO 9405912 A1 JP 3241729 S2 JP 8502569 T KR 254246 B1	18-05-1994 11-07-1996 24-05-1994 11-05-1994 05-04-1995 19-03-1998 20-08-1998 22-11-1995 16-04-1998 29-03-1995 11-05-1994 25-12-2001 26-03-1996 16-08-2000
EP 0542723	A 19-05-1993	AT 93418 T EP 0542723 A2 EP 0718046 A2 AT 143295 T AT 194511 T AU 637658 B2 AU 6789790 A BR 9006291 A CA 2031907 A1 CN 1054916 A DE 6900292 D1 DE 69028718 D1 DE 69033591 D1 DE 69033591 T2 DK 432392 T3 DK 542723 T3	15-09-1993 19-05-1993 26-06-1996 15-10-1996 15-07-2000 03-06-1993 23-07-1992 24-09-1991 13-06-1991 02-10-1991 10-09-1993 31-10-1996 17-03-2000 23-11-2000 10-01-1994 03-03-1997

page 1 of 2

INTERNATIONAL SEARCH REPORT		PCT/GB 01/04964	
Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP 0542723	A	EP 0432992 A1 ES 2030348 A5 ES 2043293 T3 ES 2092146 T3 FI 906089 A FI 931780 A FR 2655572 A1 GB 2240494 A GB 2263076 A IE 904468 A1 IL 96597 A IT 1244183 B JP 1917114 C JP 4100553 A JP 6040984 B KR 152888 B1 MX 172730 B NO 179275 B NZ 236418 A PT 86169 A RU 2051755 C1 US 5152456 A US 5261601 A ZA 9009776 A	19-06-1991 16-10-1992 16-12-1993 16-11-1996 13-06-1991 20-04-1993 14-06-1991 07-08-1991 14-07-1993 19-06-1991 12-04-1994 08-07-1994 23-03-1995 02-04-1992 01-06-1994 01-10-1998 10-01-1994 03-06-1996 23-12-1992 31-08-1992 10-01-1996 06-10-1992 16-11-1993 26-08-1992
US 5823434	A 20-10-1998	US 5938118 A	17-08-1999

page 2 of 2